CORRECTIVE: ACTION	Get into the calibration mode and select the motor type. If the error persists, notify Danninger Medical's Service Department at 1-800-225-1814.

G. Warranty Information

Danninger Medical Technology, Inc. ("Danninger") warrants to the original purchaser ("Buyer") of this DANNIFLEX 500™ (the "Unit") that the Unit will be free from defects in material or workmanship for a period of One Year from the date of original purchase. This warranty does not obligate Danninger to repair or replace a Unit not defective at the time of purchase which is damaged by accident, abuse, misuse, misapplication, or unauthorized repairs or alterations. DANNINGER MAKES NO OTHER WARRANTIES, EXPRESS OR IMPLIED (INCLUDING, WITHOUT LIMITATION, MERCHANTABILITY, FITNESS FOR PARTICULAR PURPOSE, OR AGAINST INFRINGEMENT OF ANY PATENT), EXCEPT EXPRESSLY PROVIDED HEREIN.

If the unit does not conform to this warranty, Danninger will at its option repair or replace the defective Unit. The remedy of repair or replacement is Buyer's sole and exclusive remedy and will satisfy all of Danninger's liabilities, whether based on contract, tort, product liability, strict liability, or otherwise. IN NO EVENT SHALL DANNINGER BE LIABLE FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES, NOR SHALL ITS LIABILITY IN CONNECTION WITH ANY DEFECTIVE UNIT EXCEED THE SALES PRICE OF SUCH UNIT.

For this limited warranty to apply, Buyer must provide Danninger with written notice of a claimed defect within thirty days after its discovery, but not later than the expiration date of the warranty term. Within reasonable time following receipt of such notice, Danninger will advise Buyer of the disposition of the Unit. Unless expressly authorized in writing, the defective Unit must be returned to Danninger for coverage. Danninger reserves the right to inspect the Unit to determine whether the claimed defect is within the coverage of this limited warranty.

H. Ordering Replacement Parts

To order parts, simply call a Danninger customer service representative, toll free at 1-800-225-1814, or (614)-276-8267. It would be helpful to our staff if you would have the Danninger part number, your customer number, and a purchase order number available when placing the call.

I. Returning your unit to the factory for repair

To return your unit to Danninger Medical Technology for repair, simply pack your unit in its original carton it to:

Danninger Medical Technology
Attn.: Technical Service
4140 Fisher Road
Columbus, OH 43228-1607

Please enclose a note with the following information:

1) Bill to Address
2) Ship to Address
3) A purchase order number (for non-warranty repairs) with the understanding that all repairs less than $350 will be billed under this purchase order without acquiring an approval of estimate.
4) Name and phone number of person to contact for estimate approval (for repairs greater than $350) or questions concerning the repair.
5) Brief description of the problem.

J. Returning your unit to the factory for credit

Your unit may be returned to Danninger Medical Technology for credit for the following reasons:

1) Failure of unit to meet performance expectations within the warranty period.
2) Mechanical or electrical failure within the warranty period.
3) A catastrophic failure regardless of the warranty status of your unit.

In order to return your unit for credit you must receive a Return Authorization (RA #) from our Customer Service Department. You can get this number by calling a customer service representative at 1-800-225-1814 or (614) 276-8267. This number should be written clearly on the box with your returned unit.

K. Receiving Technical / Educational Support:

We invite you to call Danninger Medical Technology, toll free at 1-800-225-1814, if you have any problems operating or servicing your unit.

DANNIFLEX 500

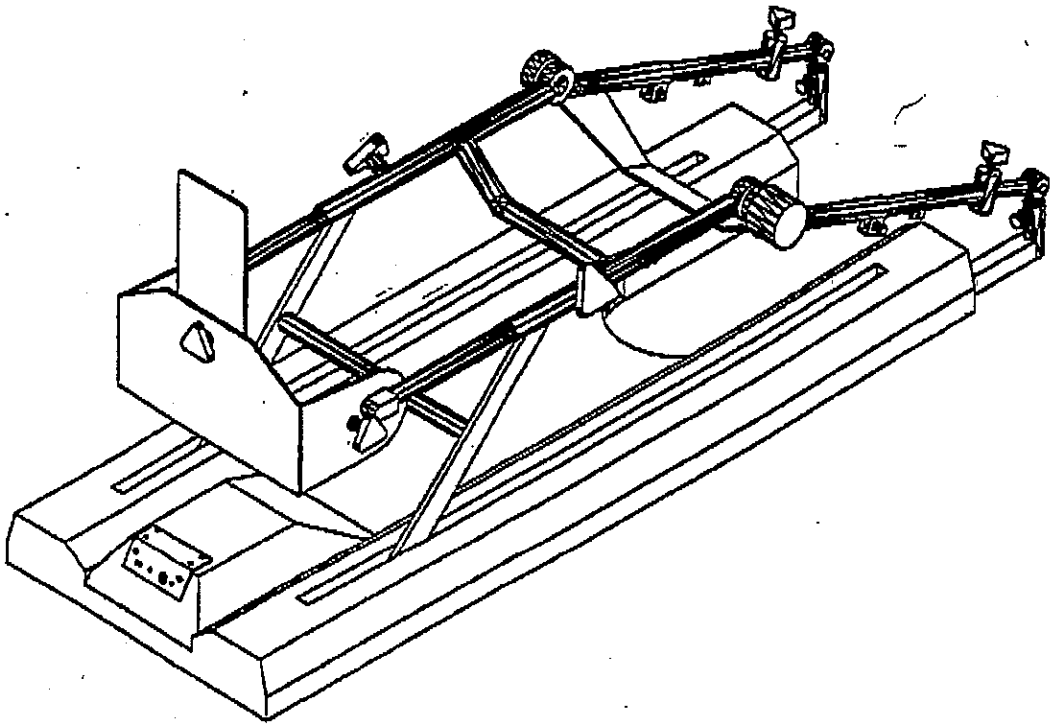

EXPLODED VIEW DIAGRAMS and PARTS LISTS

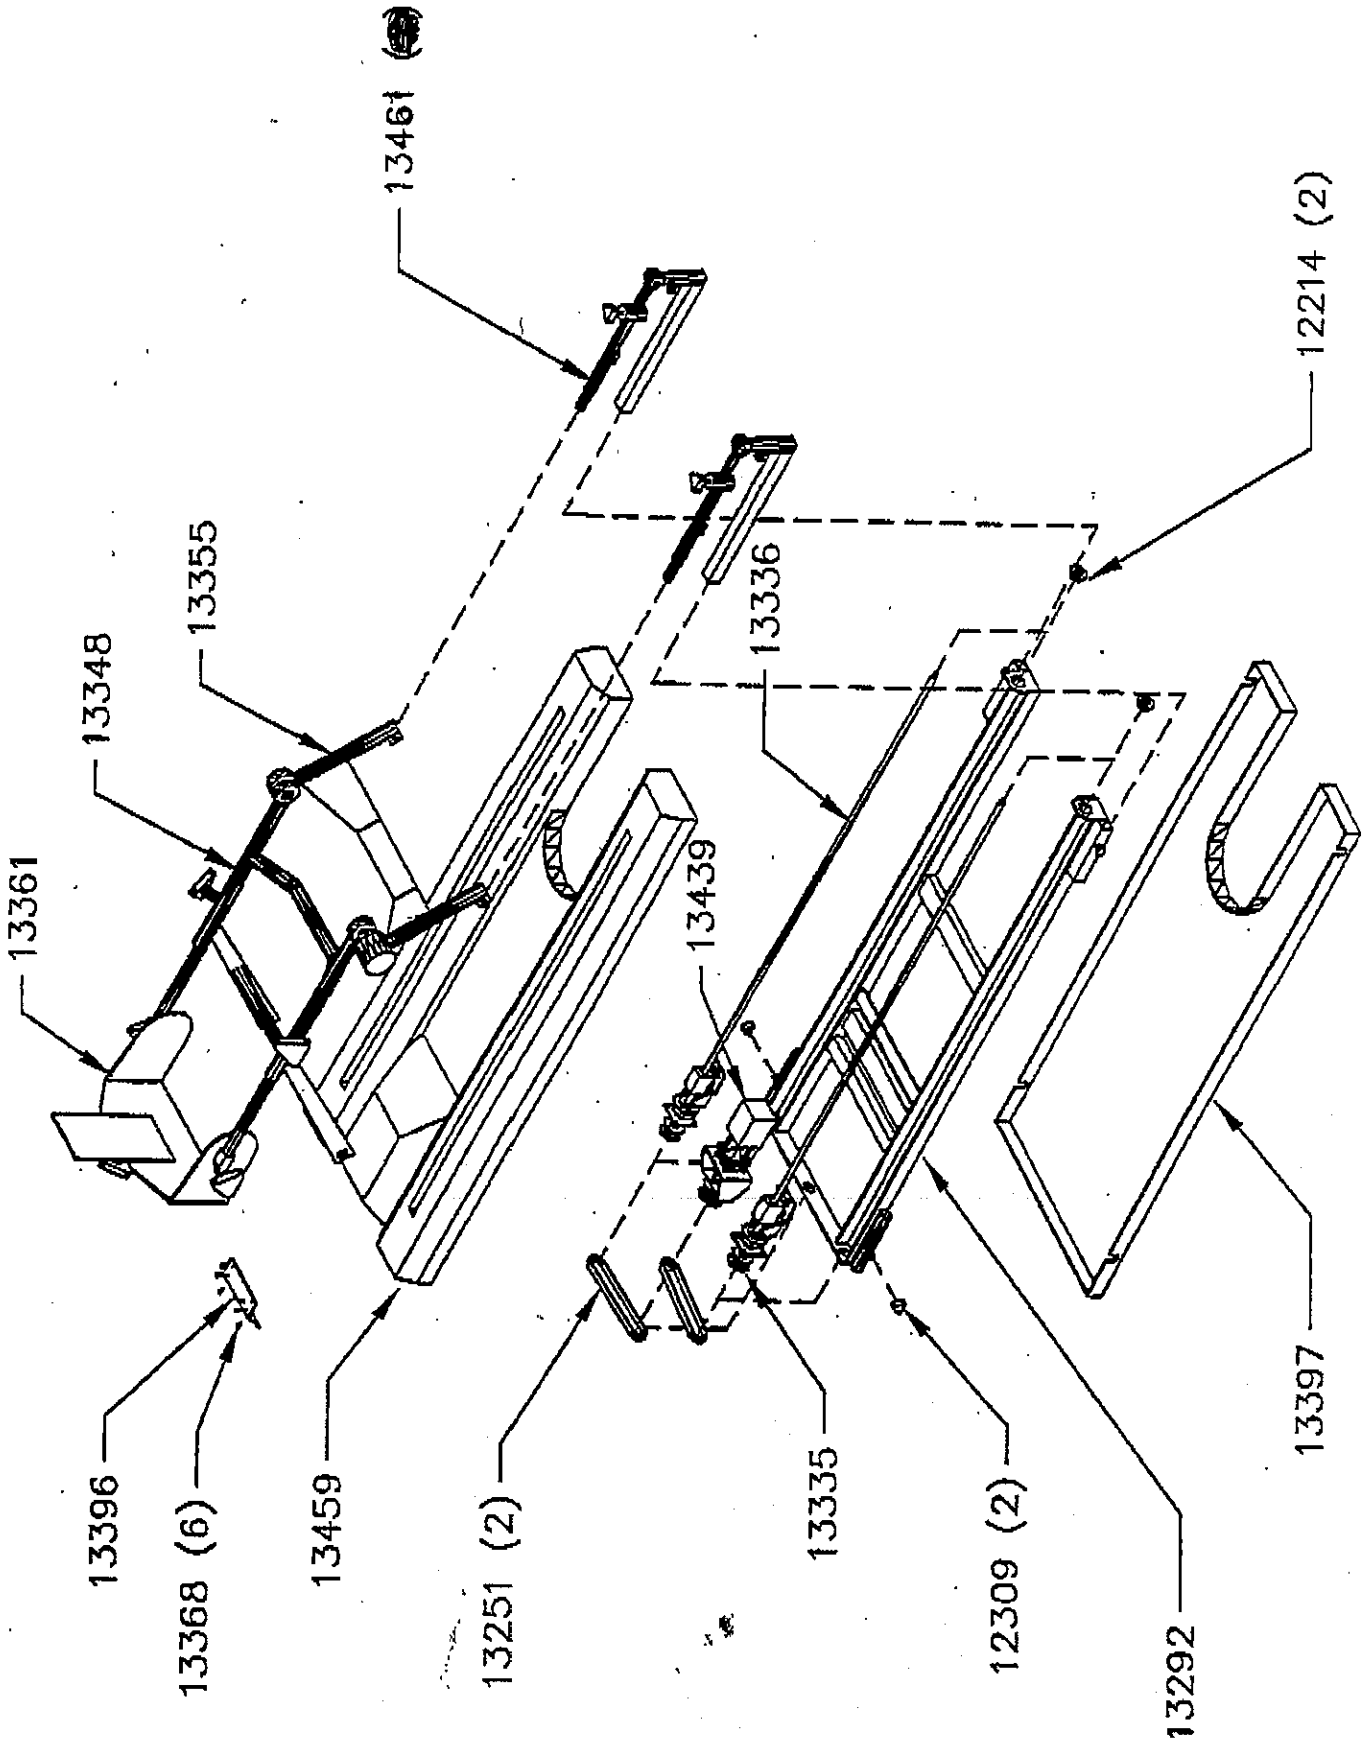
13461
12214 (2)
13355
13348
13336
13361
13439
13396
13368 (6)
13459
13251 (2)
13335
12309 (2)
13292
13397

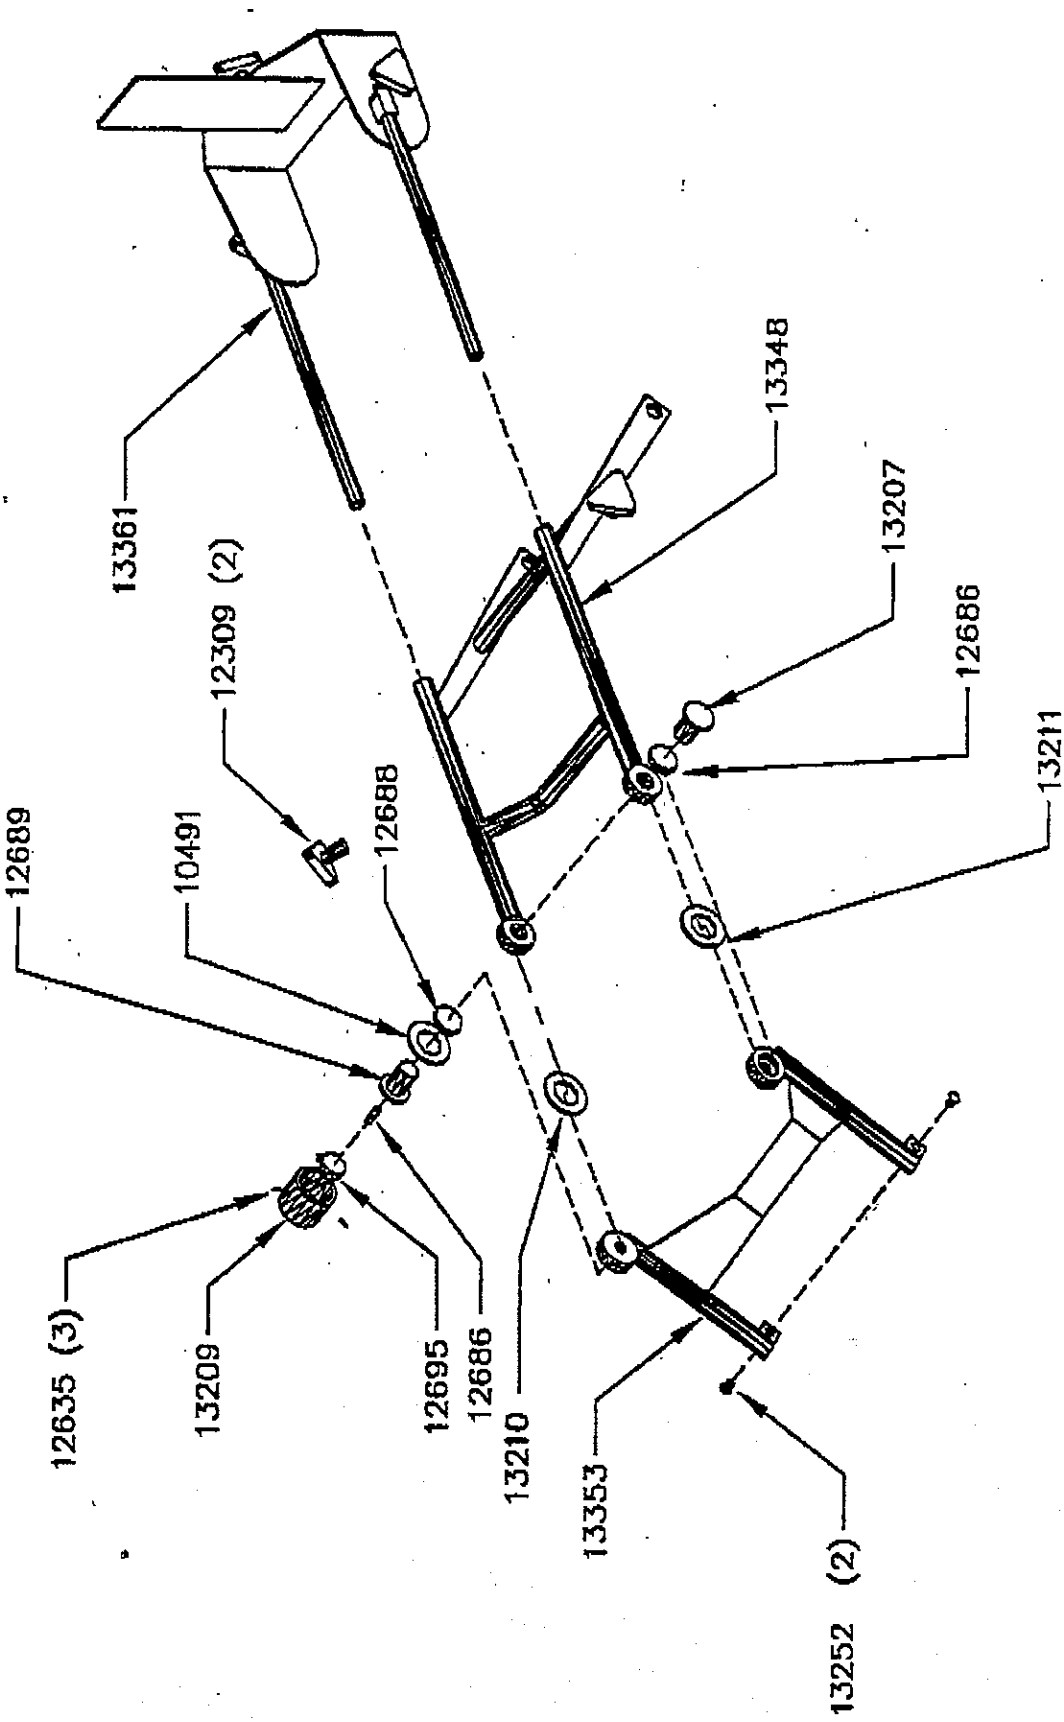
13361
12309 (2)
12689
10491
12688
12635 (3)
13209
12695
12686
13210
13353
13252 (2)
13348
13207
12686
13211

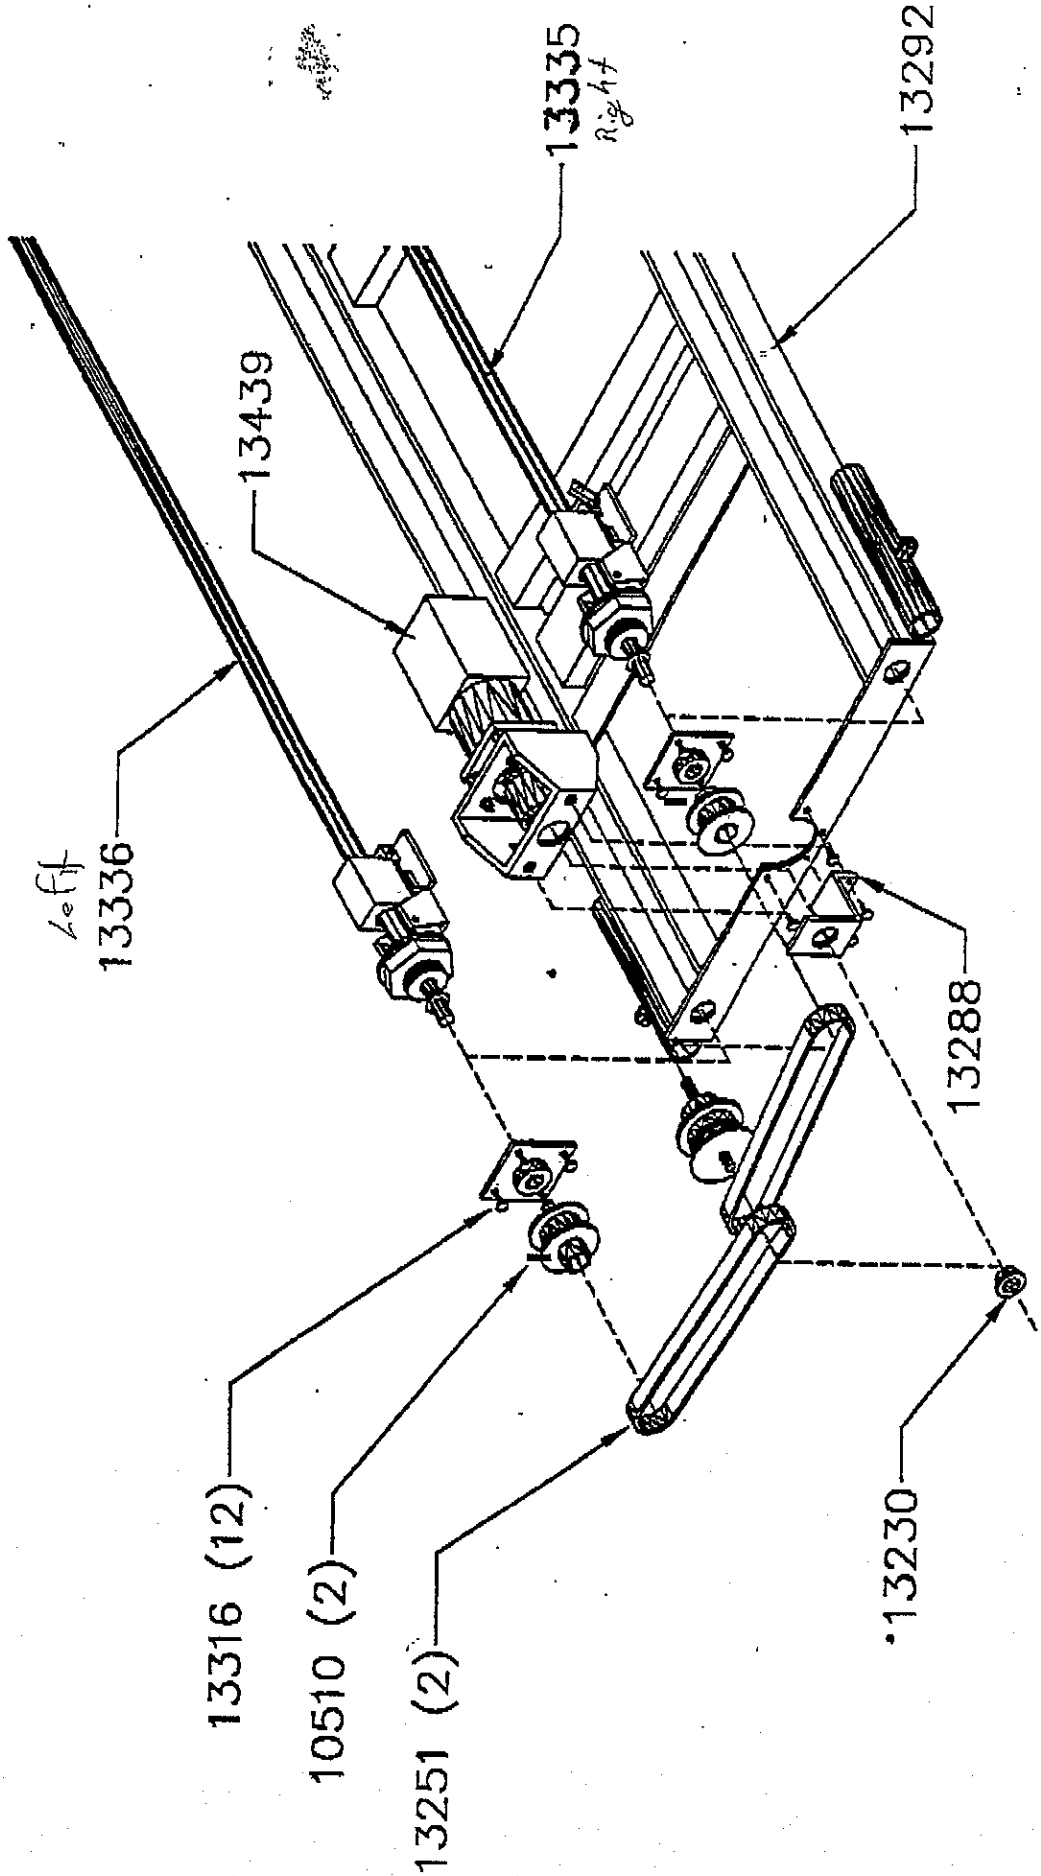
13335
Right
13292
13439
Left
13336
13288
13316 (12)
10510 (2)
13251 (2)
*13230

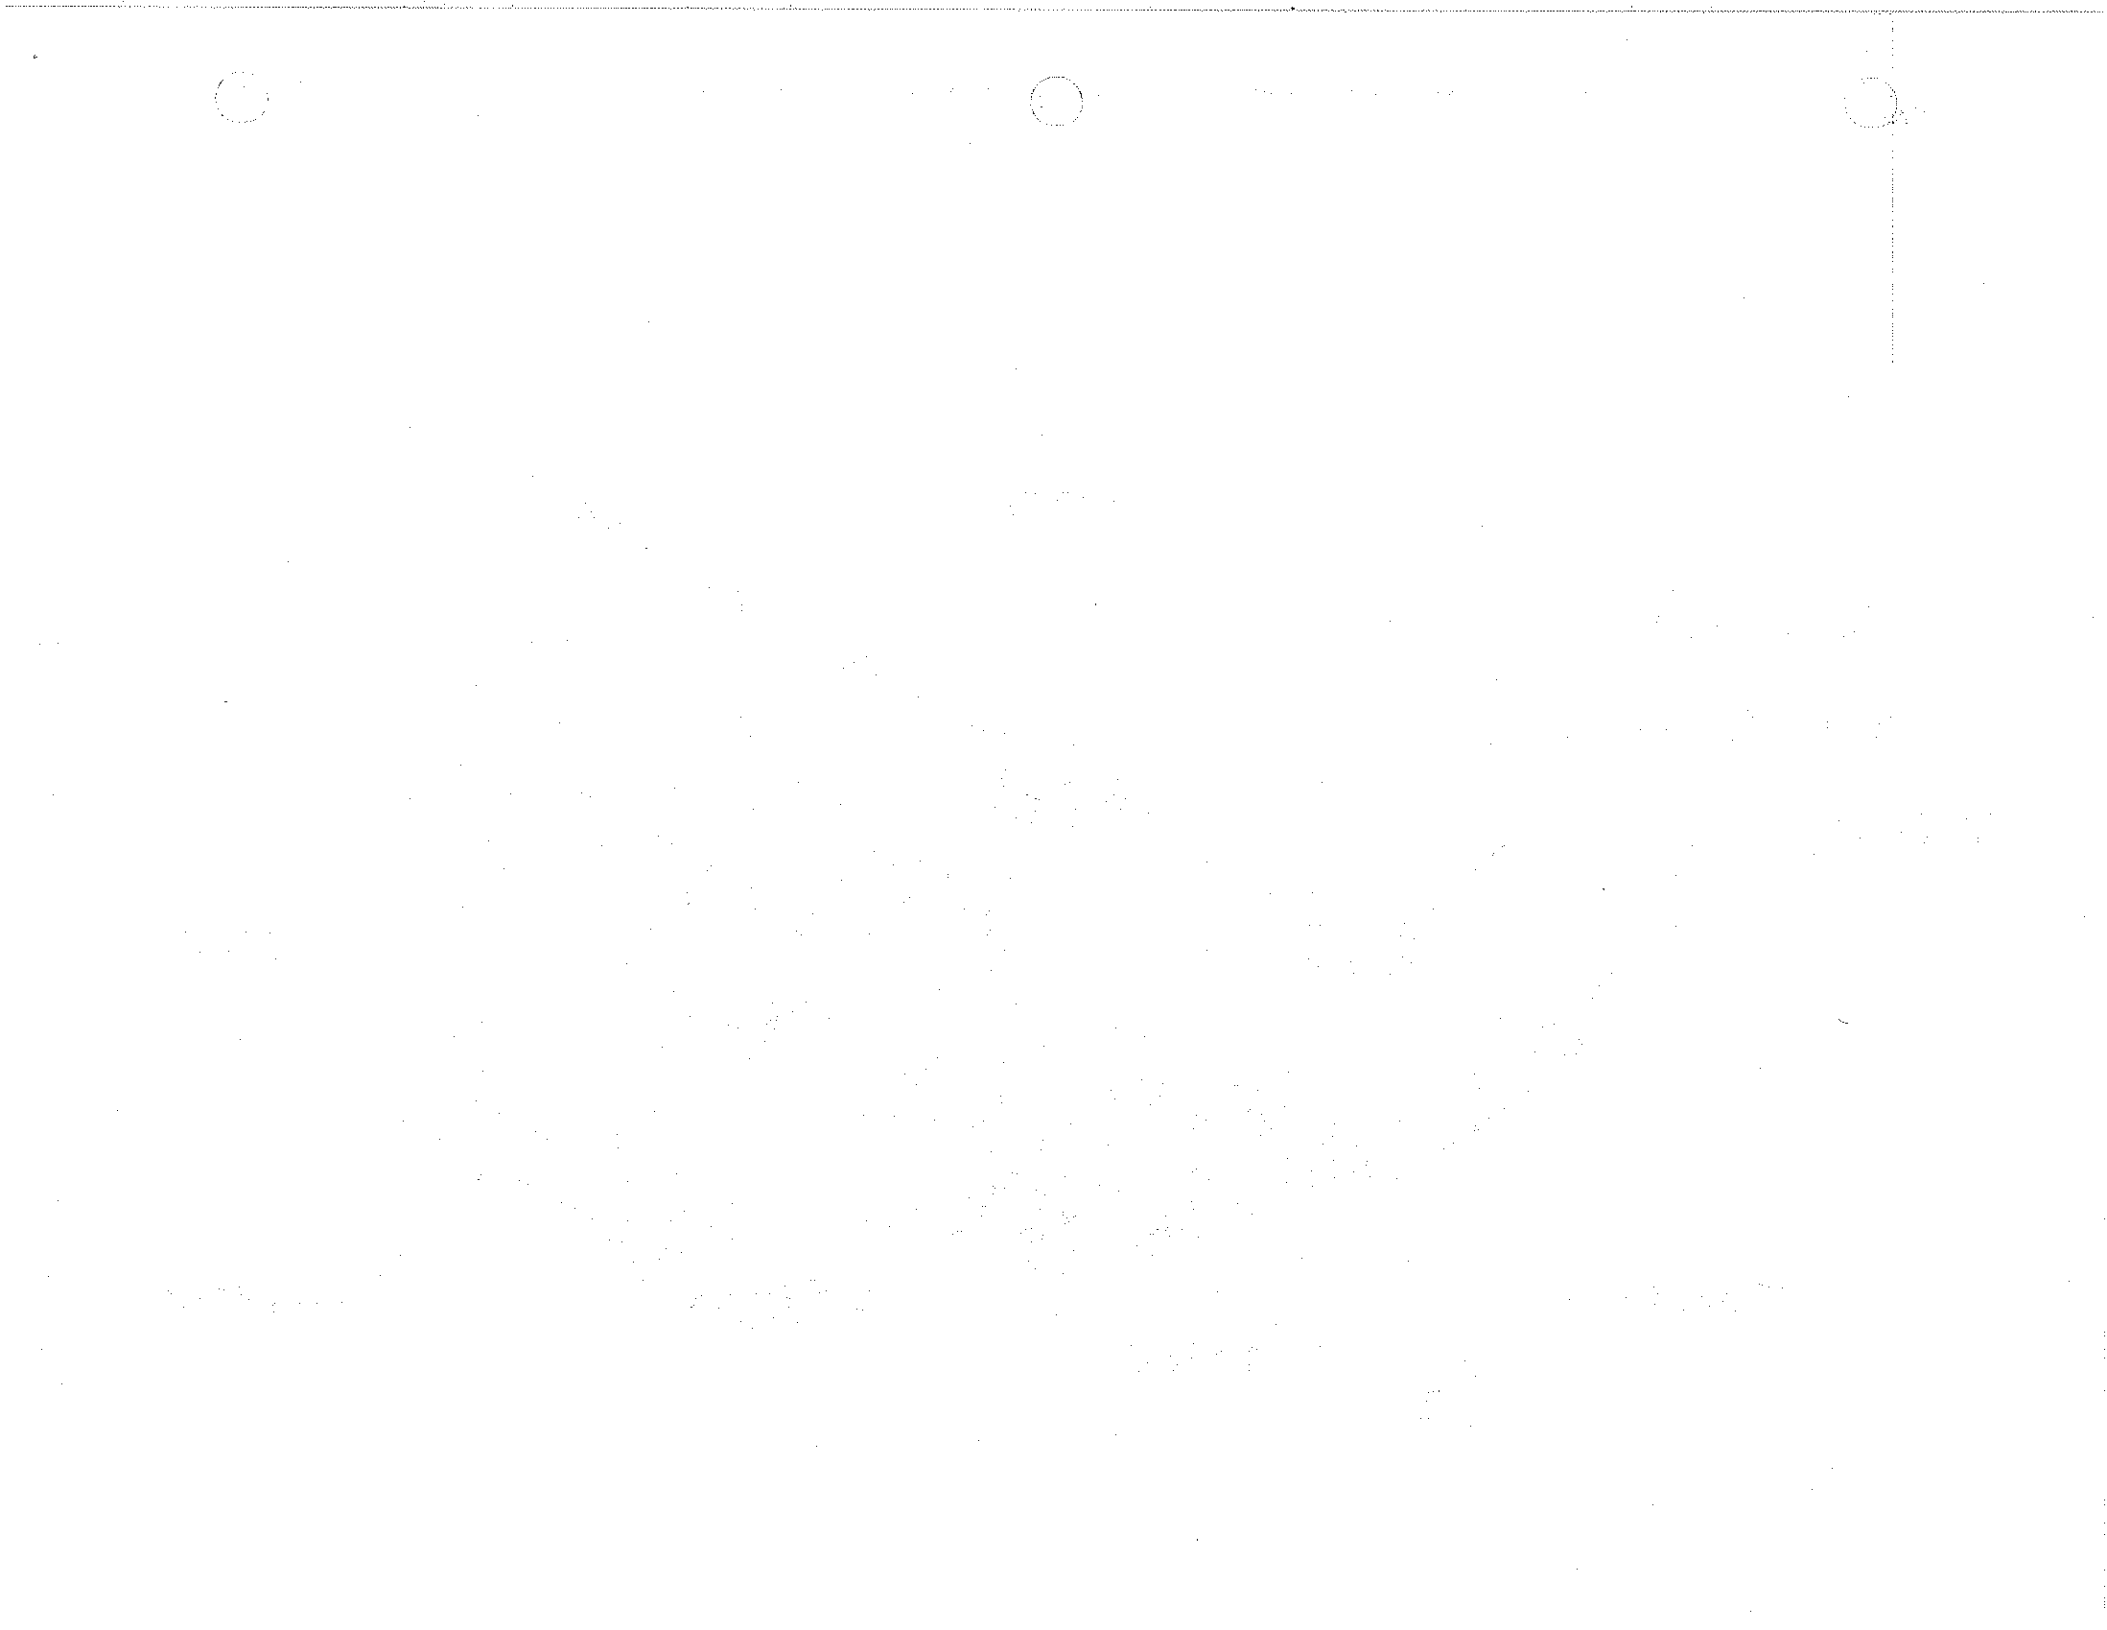

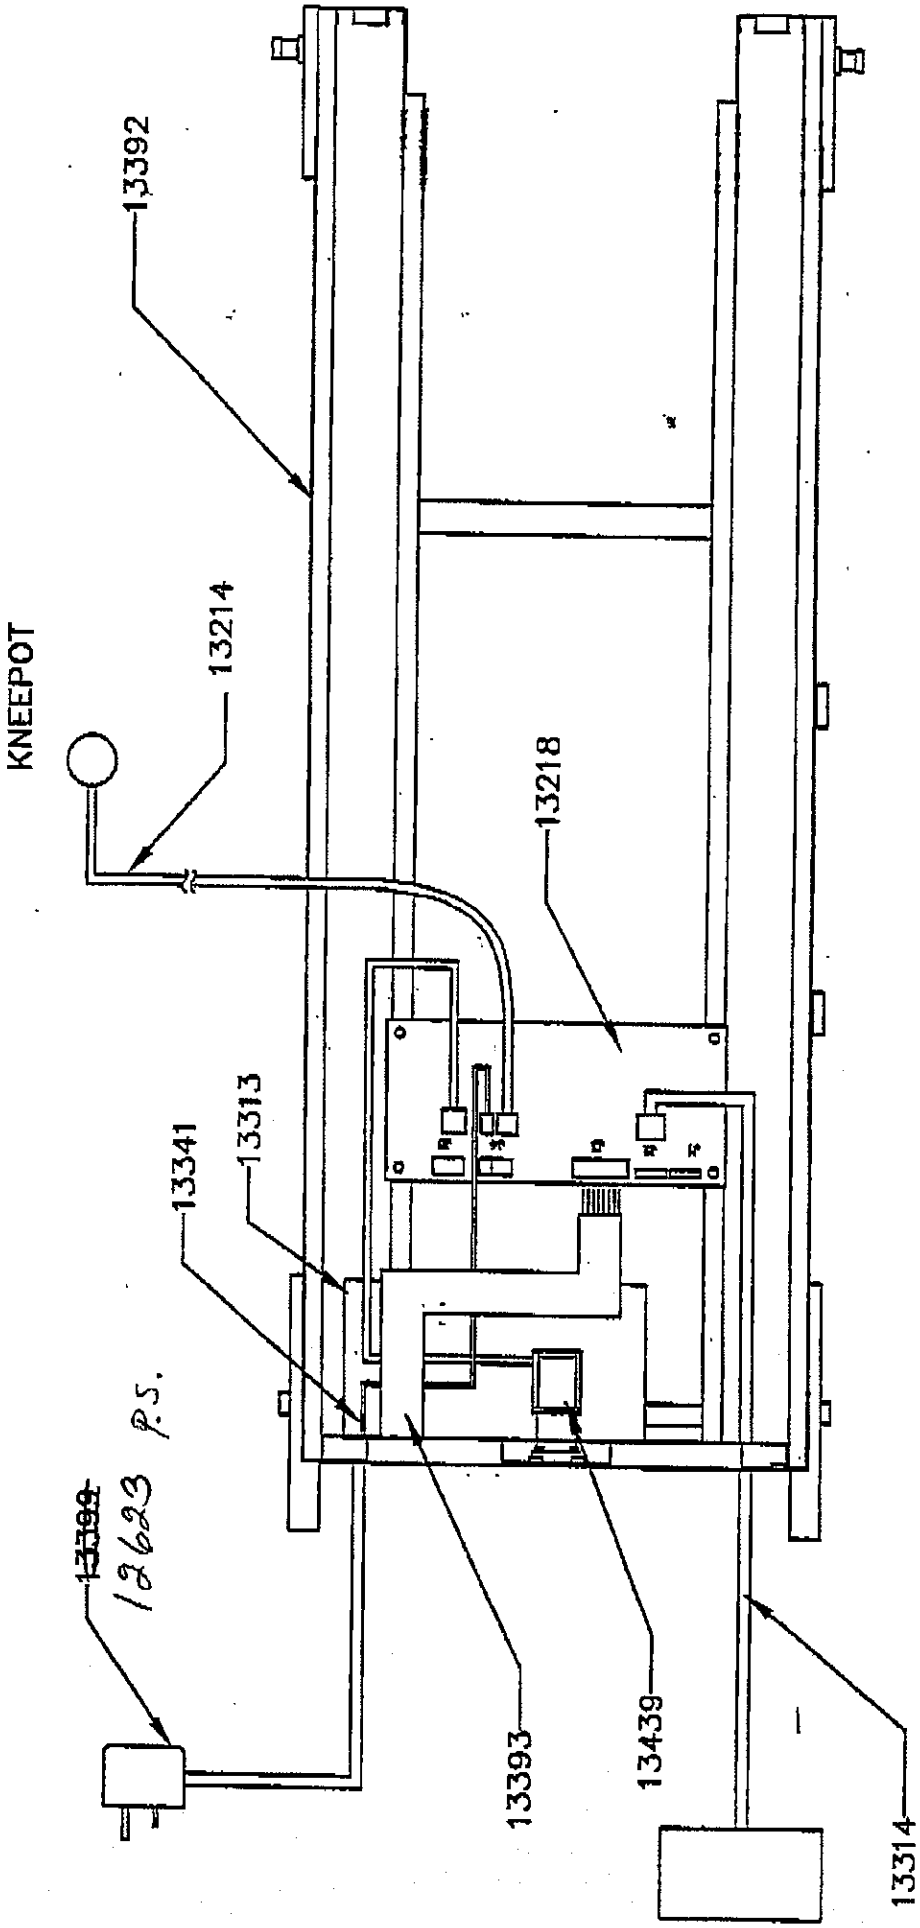
13392
13214
KNEEPOT
13218
13313
13341
P.S.
12623
13393
13439
13314

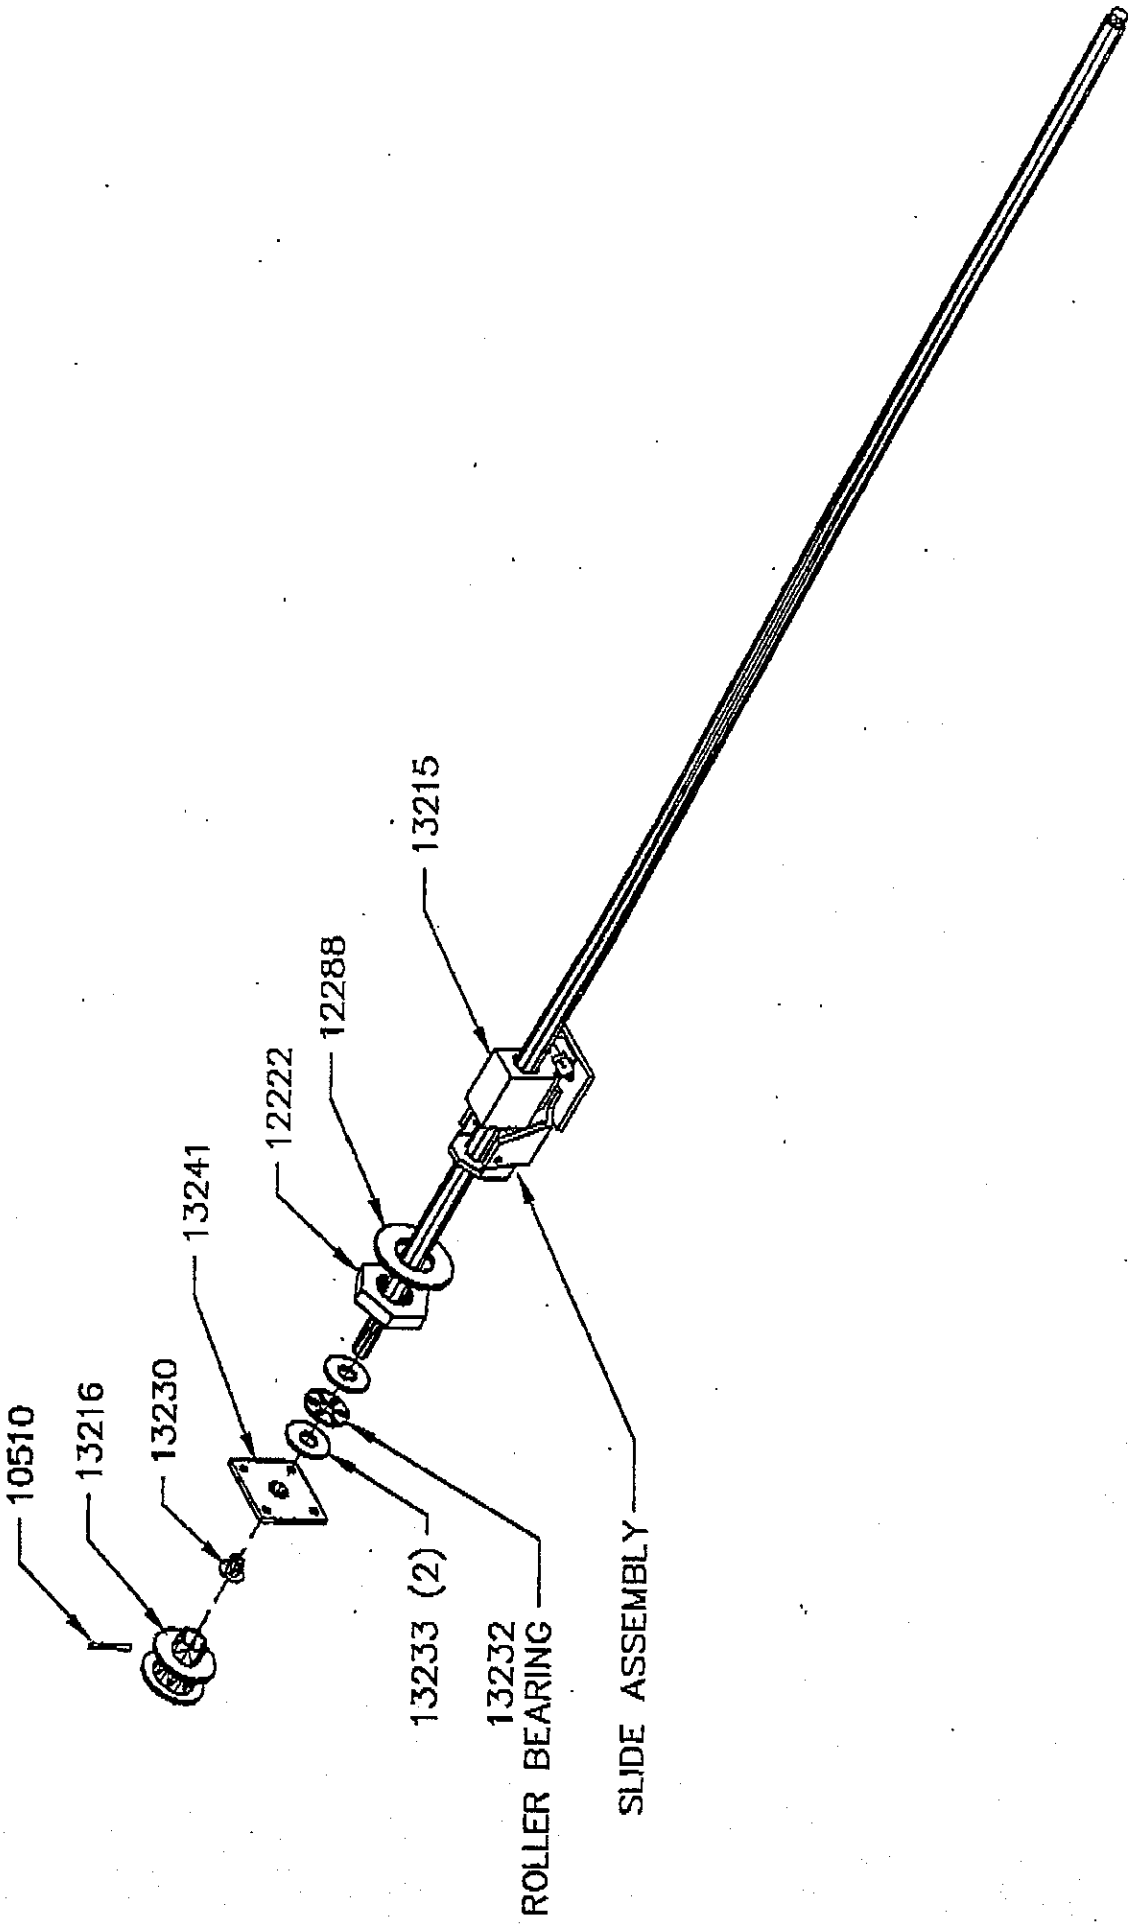
10510
13216
13230
13241
12222
12288
13215
13233 (2)
13232
ROLLER BEARING
SLIDE ASSEMBLY

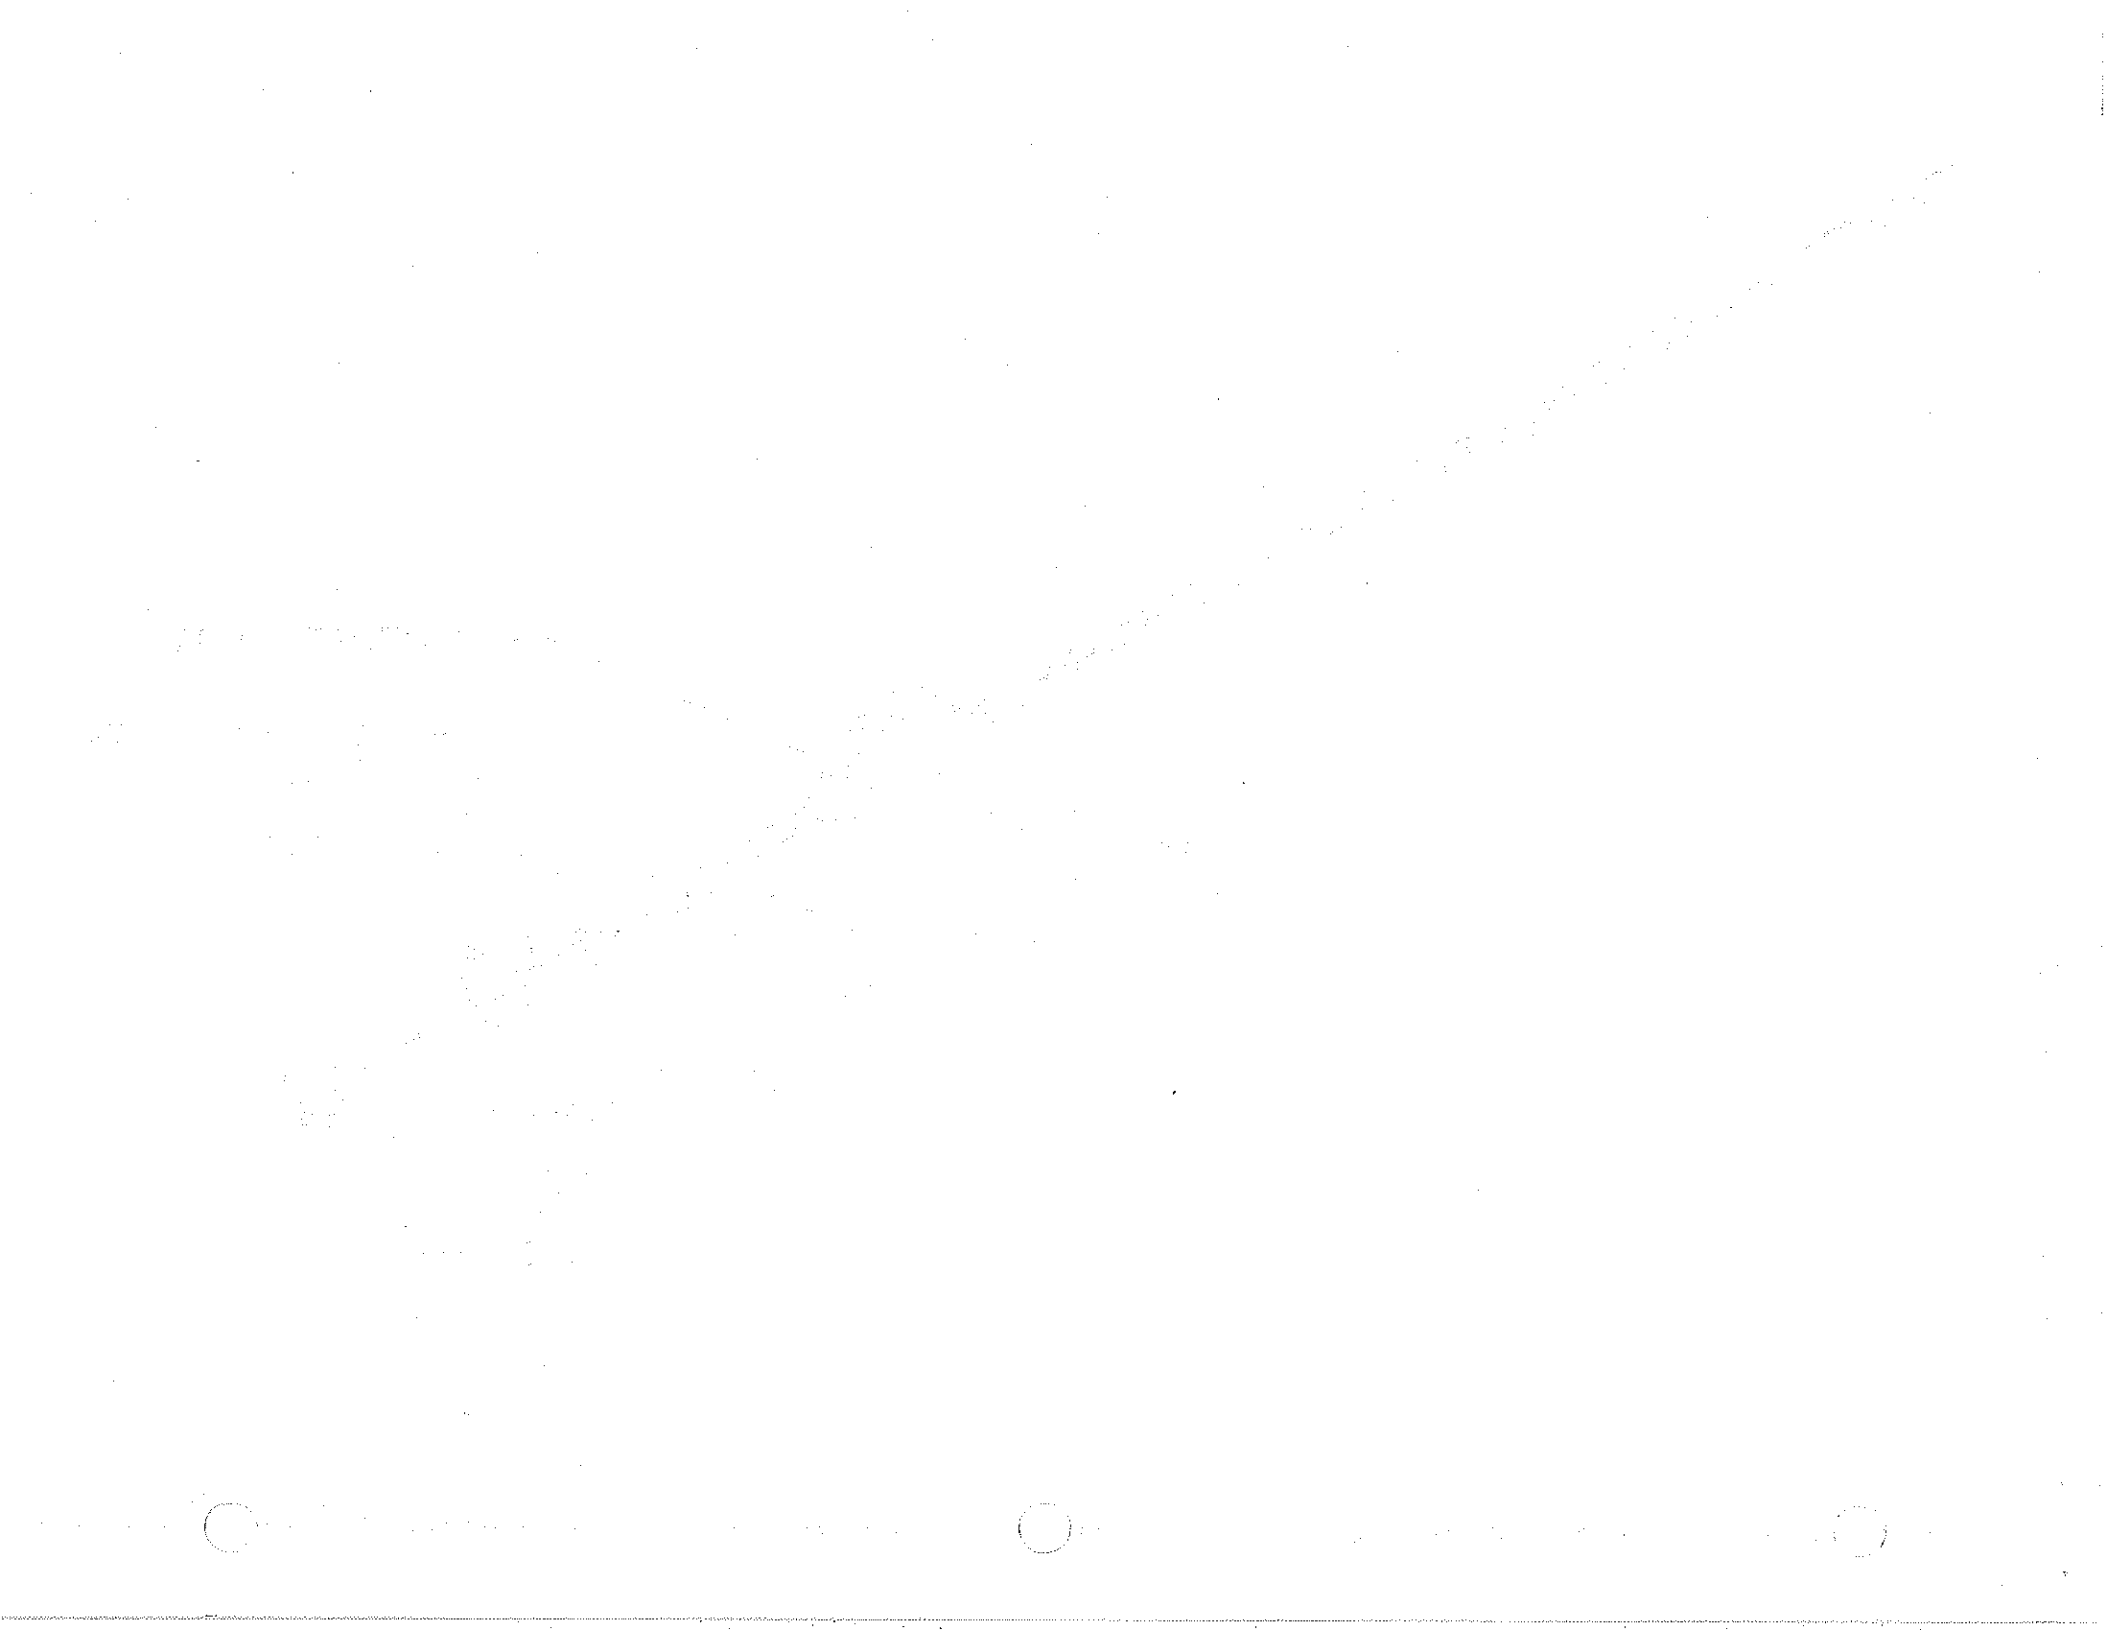

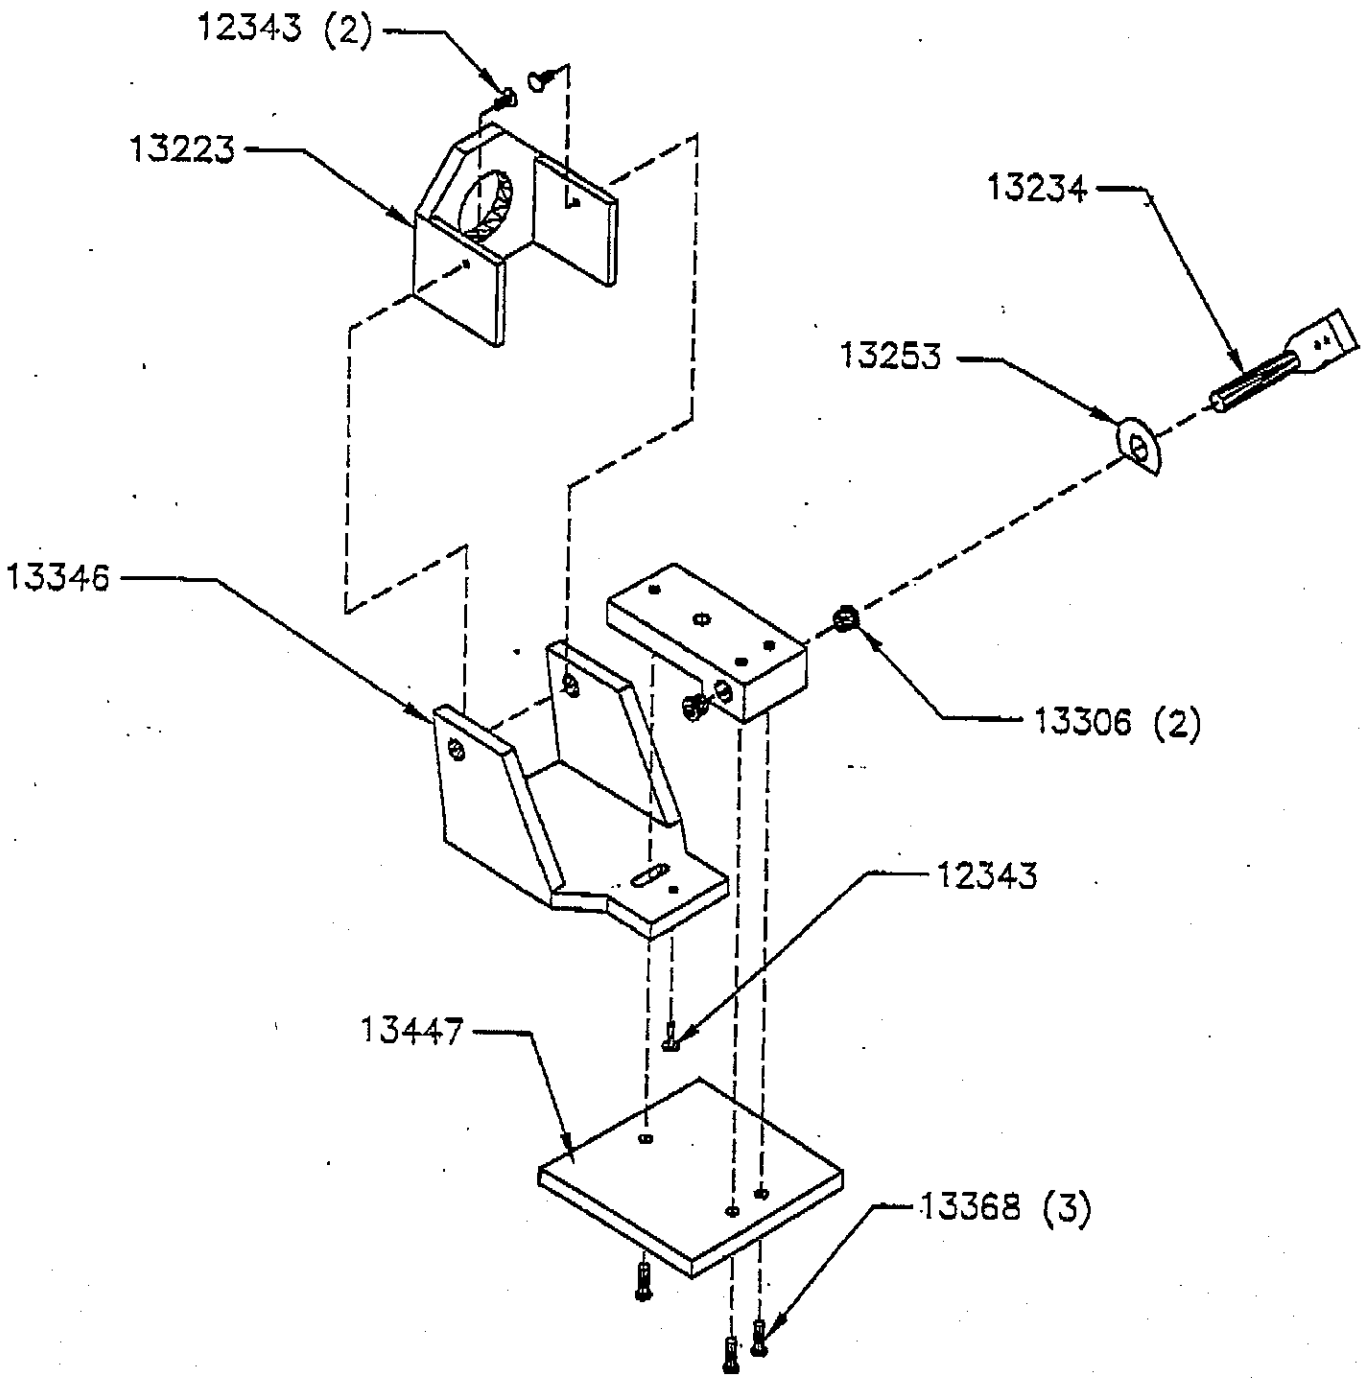
12343 (2)
13223
13234
13253
13346
13306 (2)
12343
13447
13368 (3)

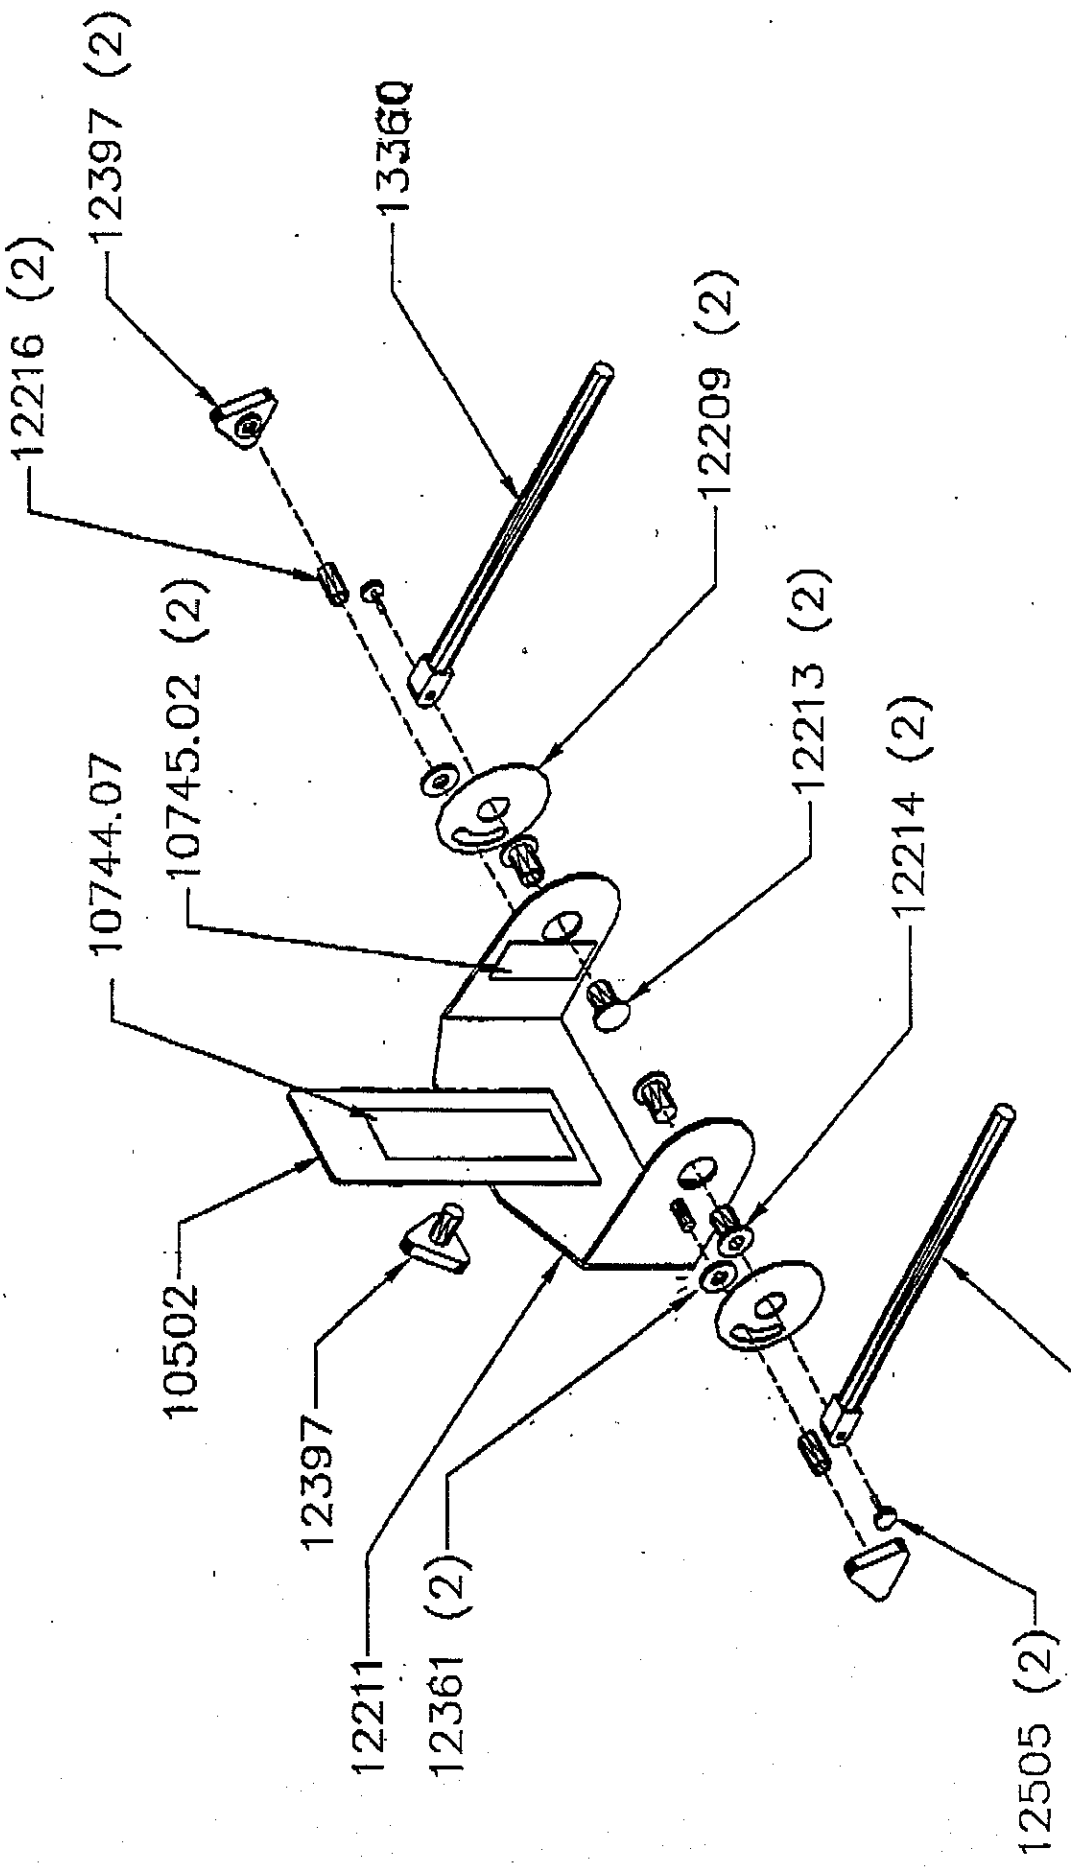
12216 (2)
12397 (2)
13360
12209 (2)
10744.07
10745.02 (2)
12213 (2)
12214 (2)
10502
12397
12211
12361 (2)
12505 (2)

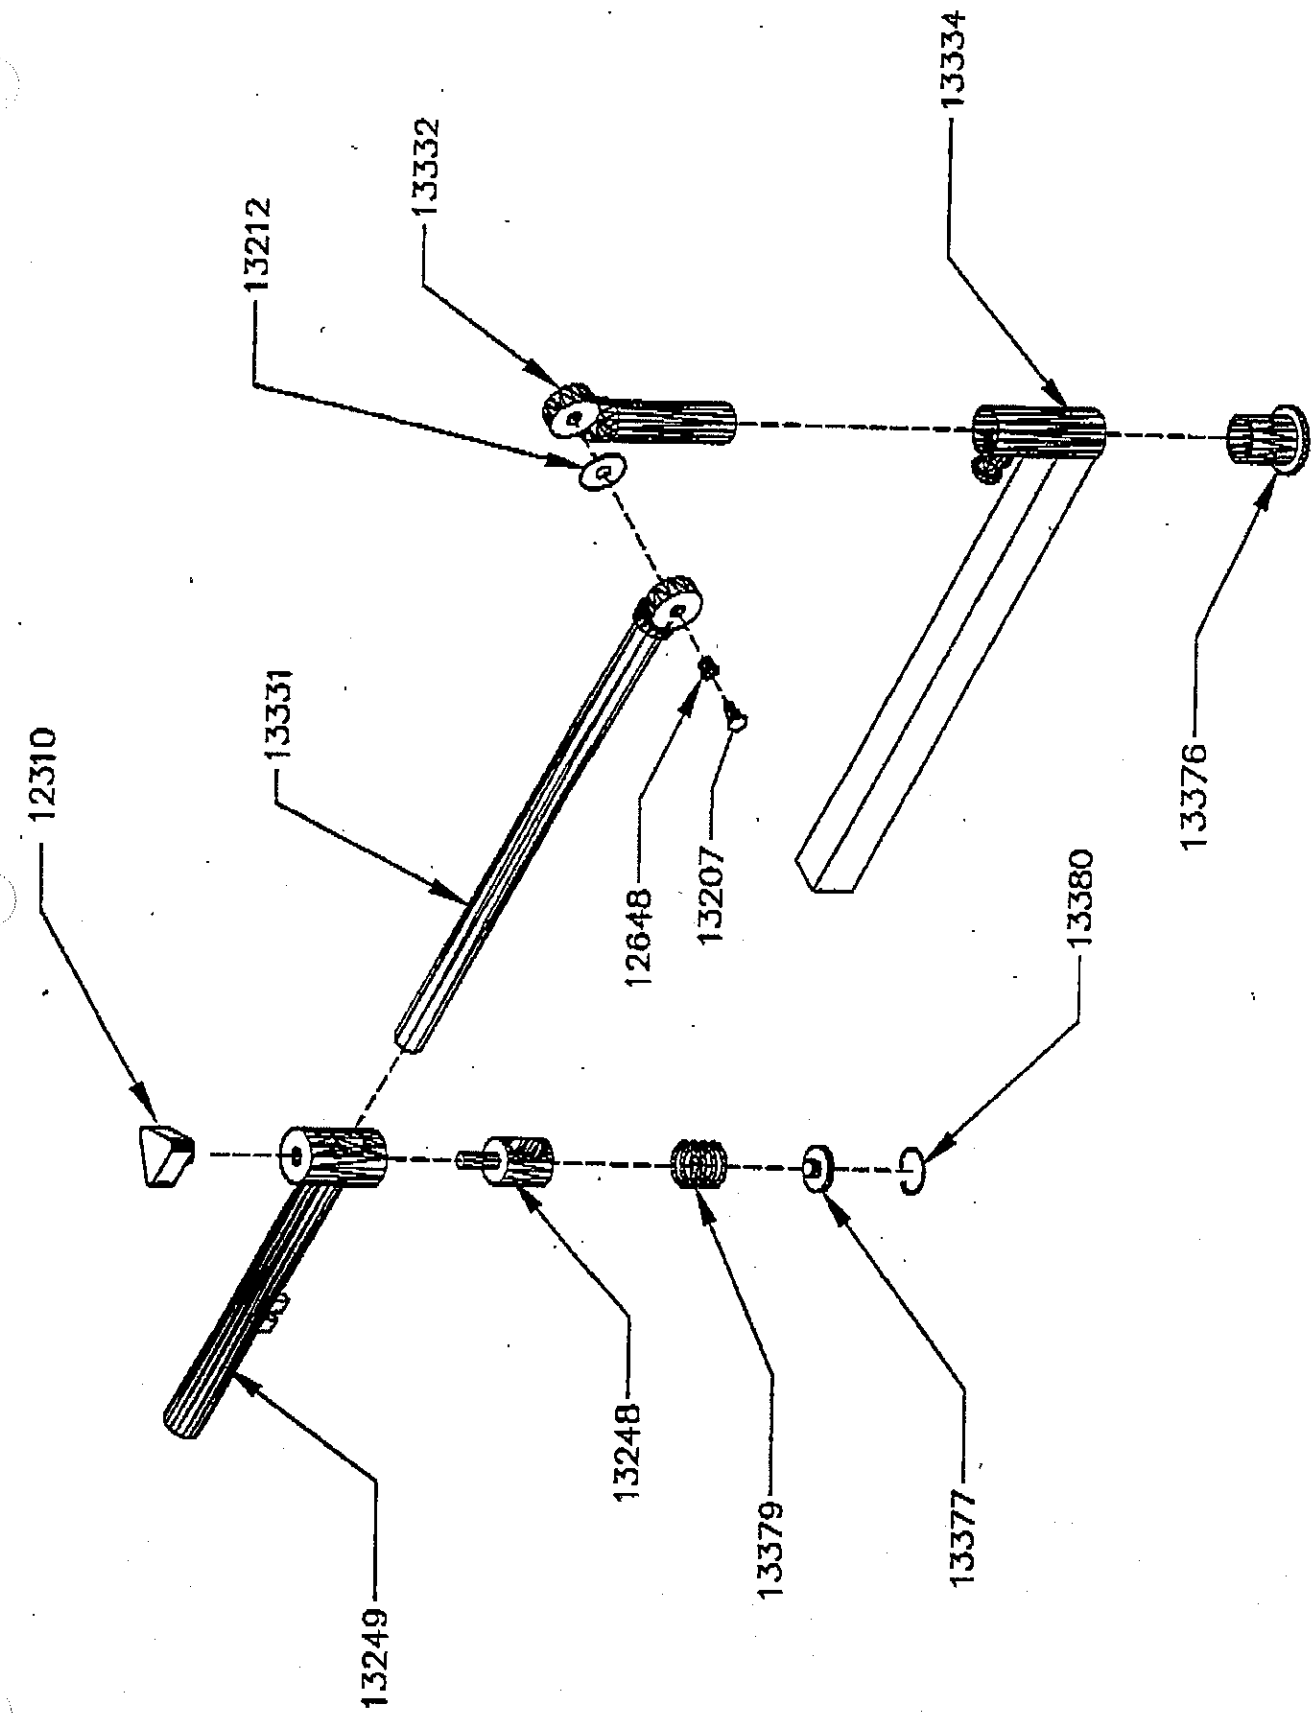
13334
13332
13212
13376
13331
12310
12648
13207
13380
13248
13379
13377
13249

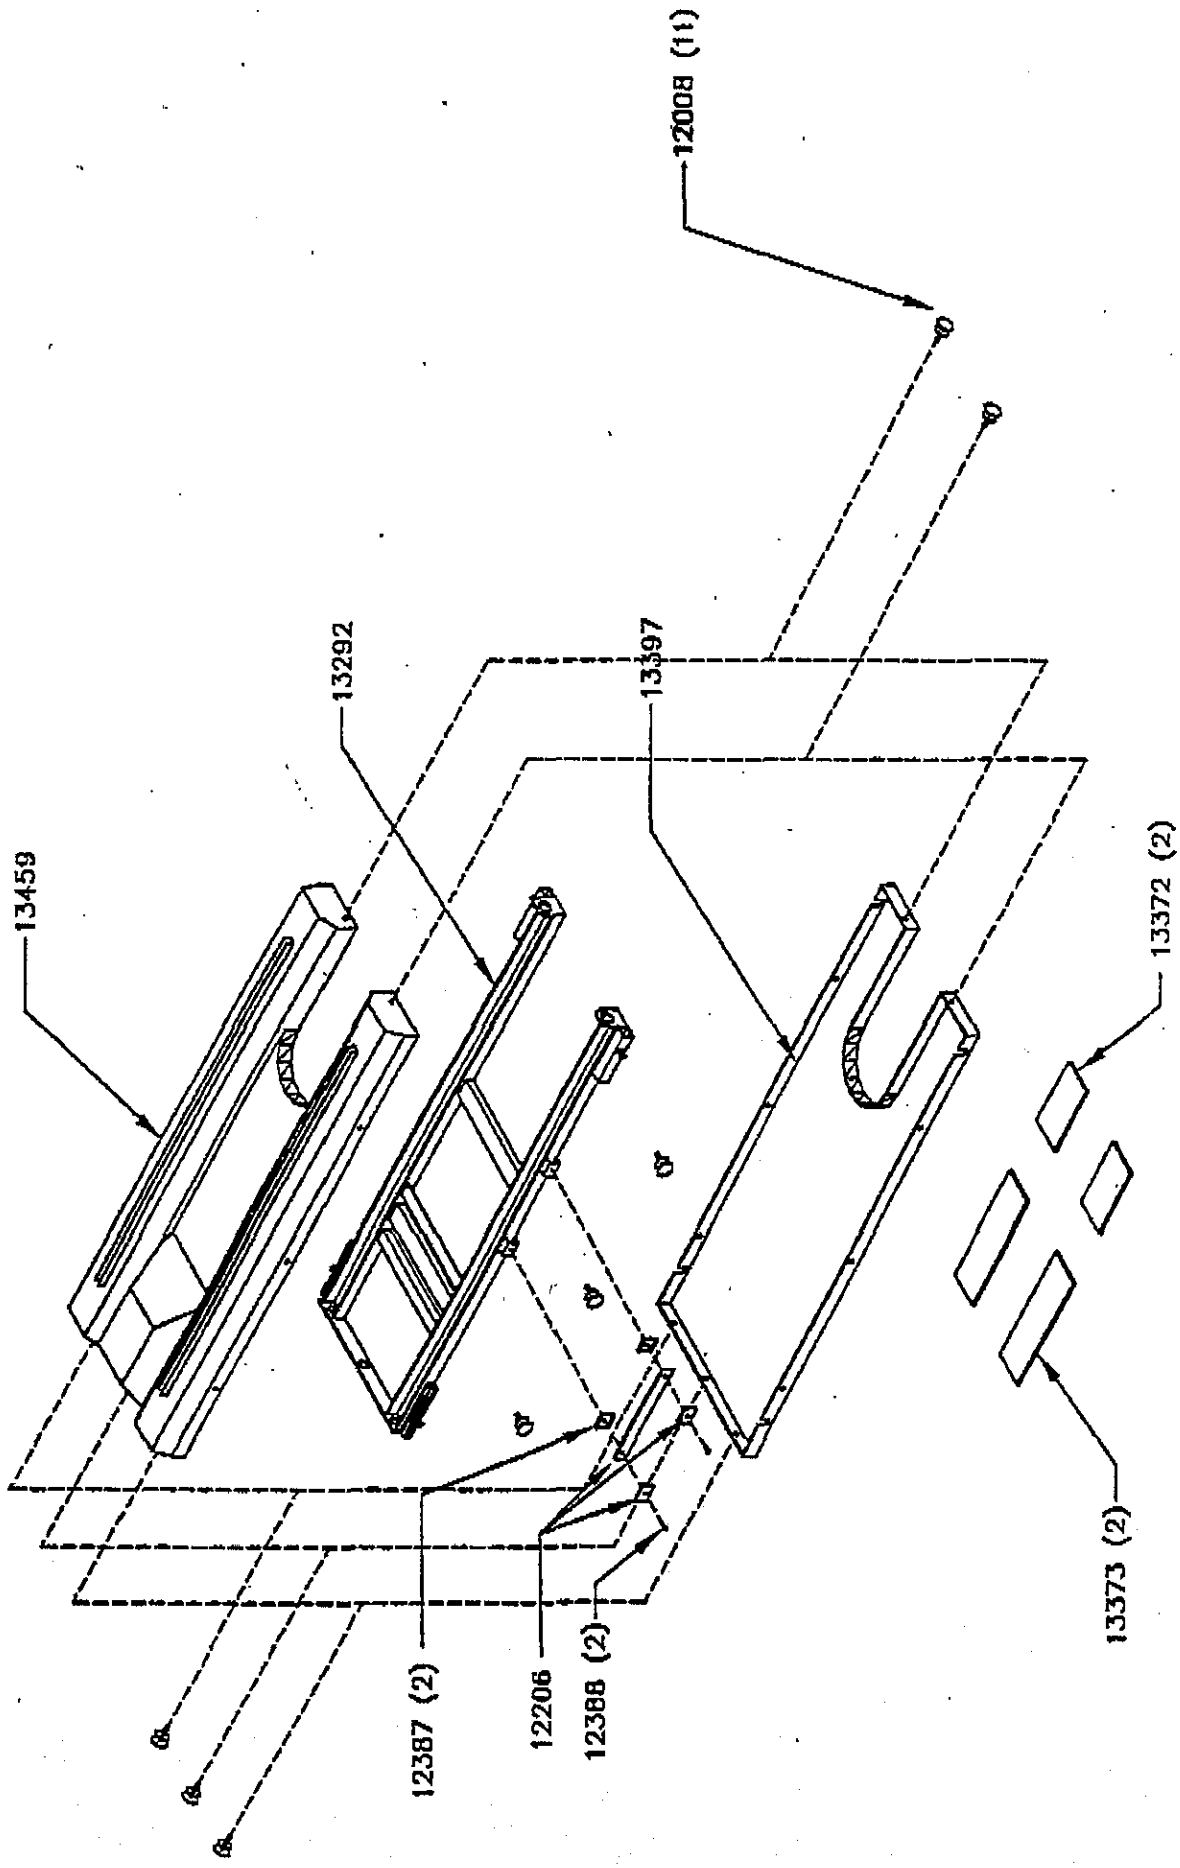
12008 (11)
13292
13397
13459
13372 (2)
13373 (2)
12387 (2)
12206
12388 (2)

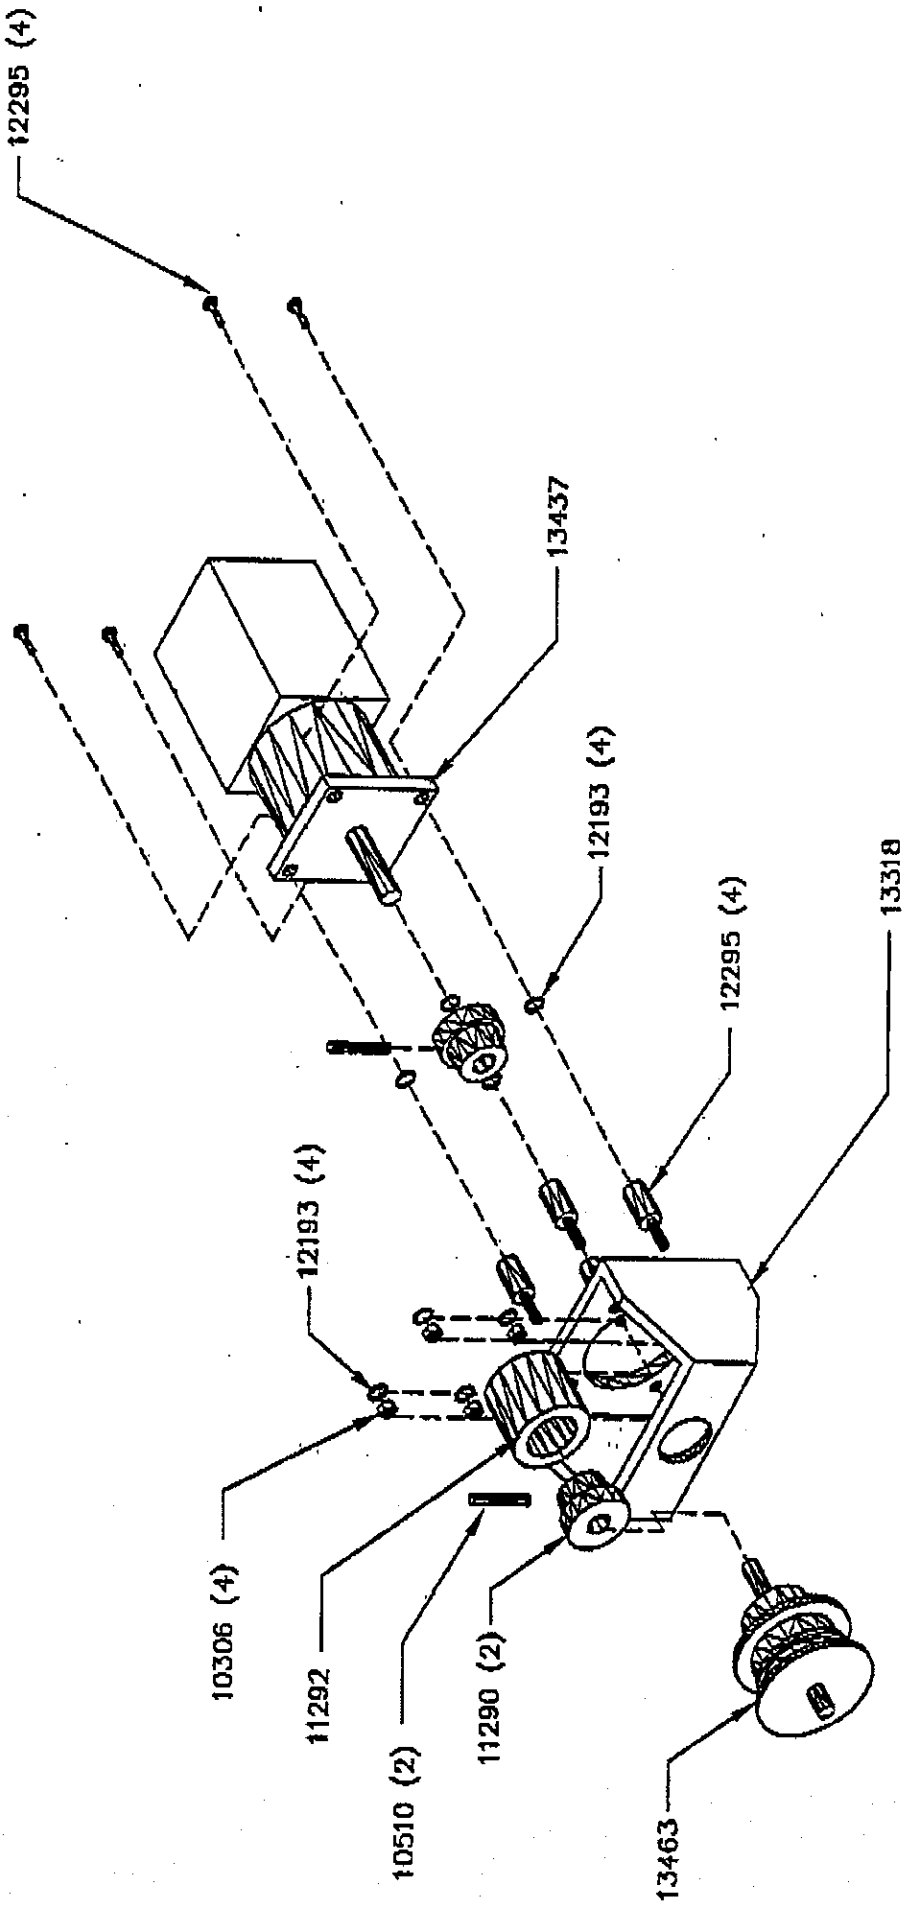

13439 KIT MOTOR ASSY

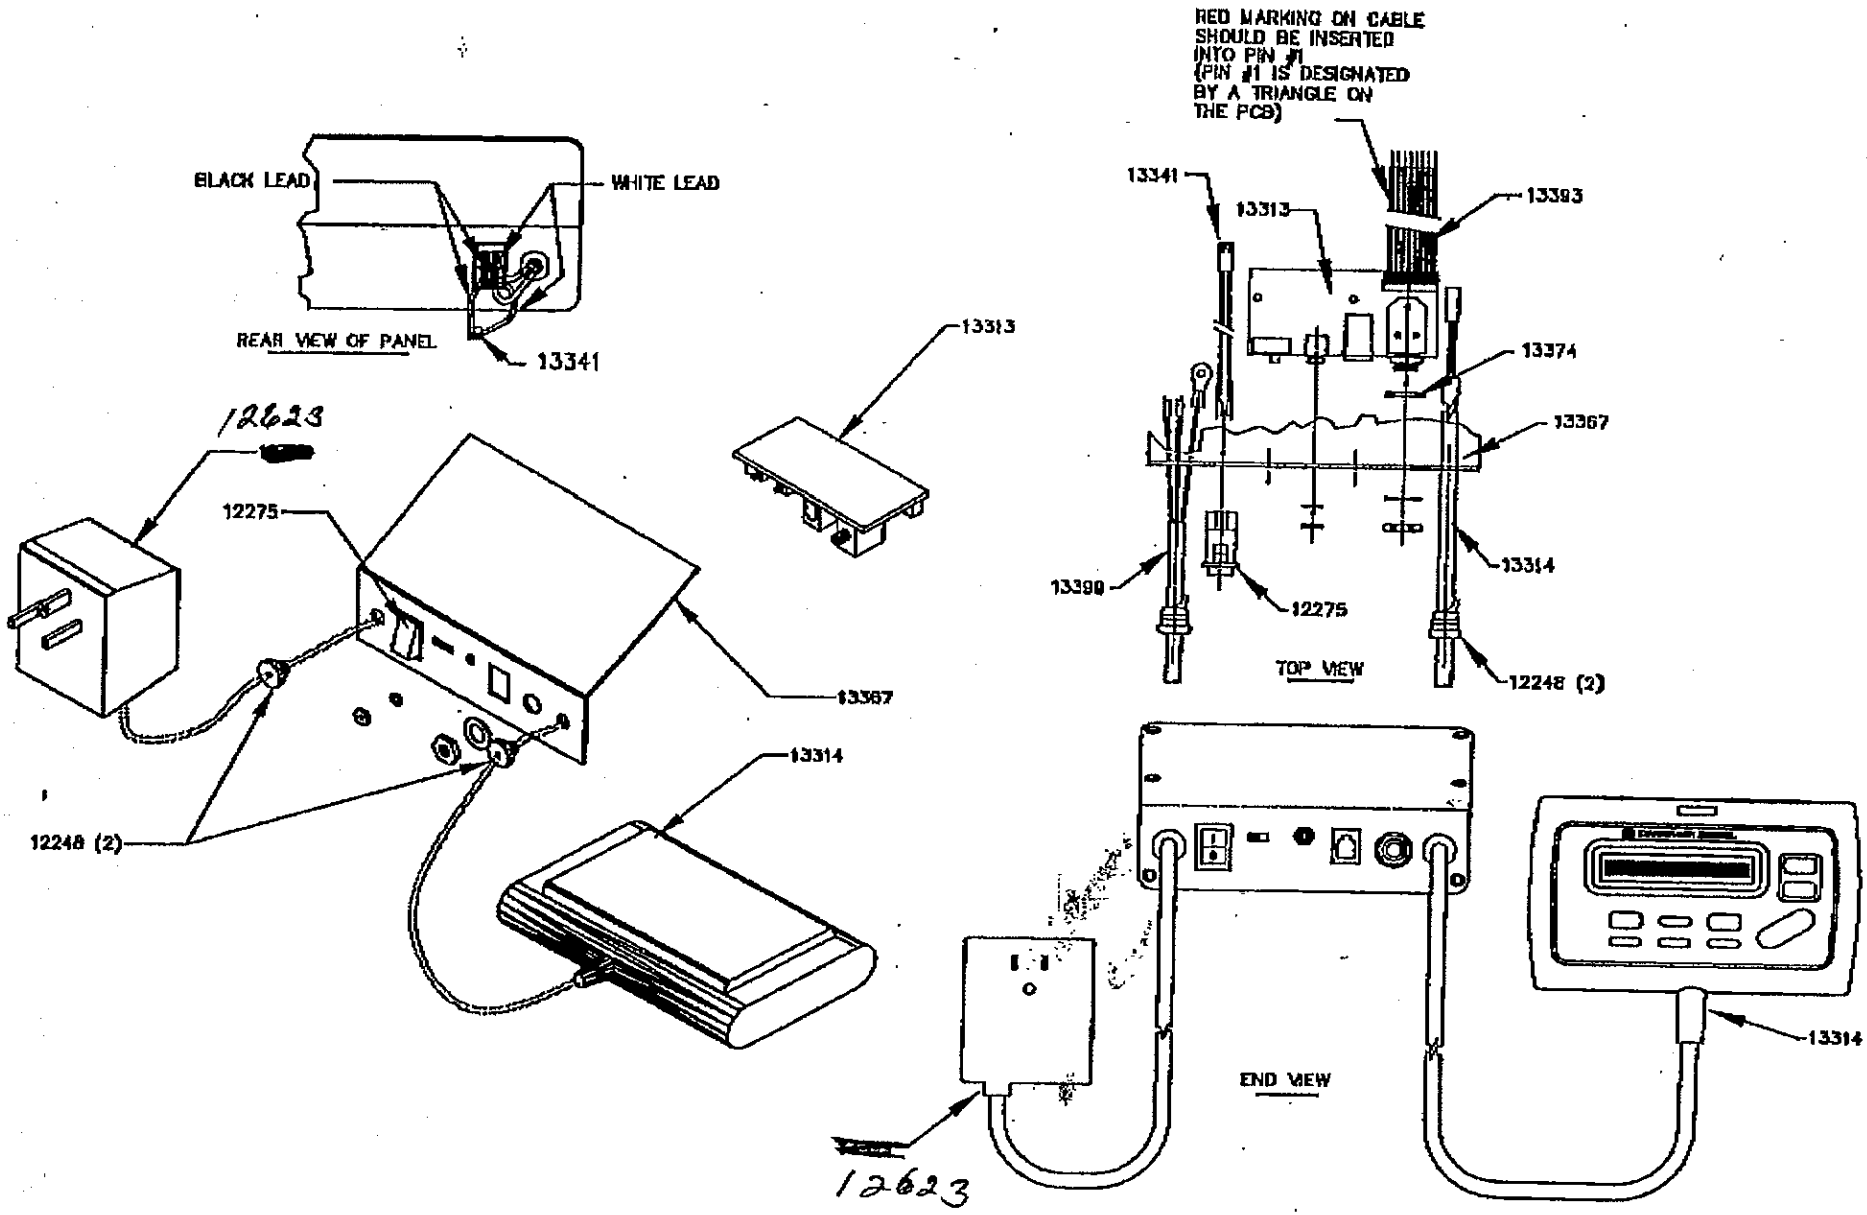
BLACK LEAD
WHITE LEAD
REAR VIEW OF PANEL
13341
13313
12623
12275
13367
13314
12248 (2)
12623
RED MARKING ON CABLE SHOULD BE INSERTED INTO PIN #1 (PIN #1 IS DESIGNATED BY A TRIANGLE ON THE PCB)
13341
13313
13393
13374
13367
13314
13390
12275
TOP VIEW
12248 (2)
END VIEW
13314

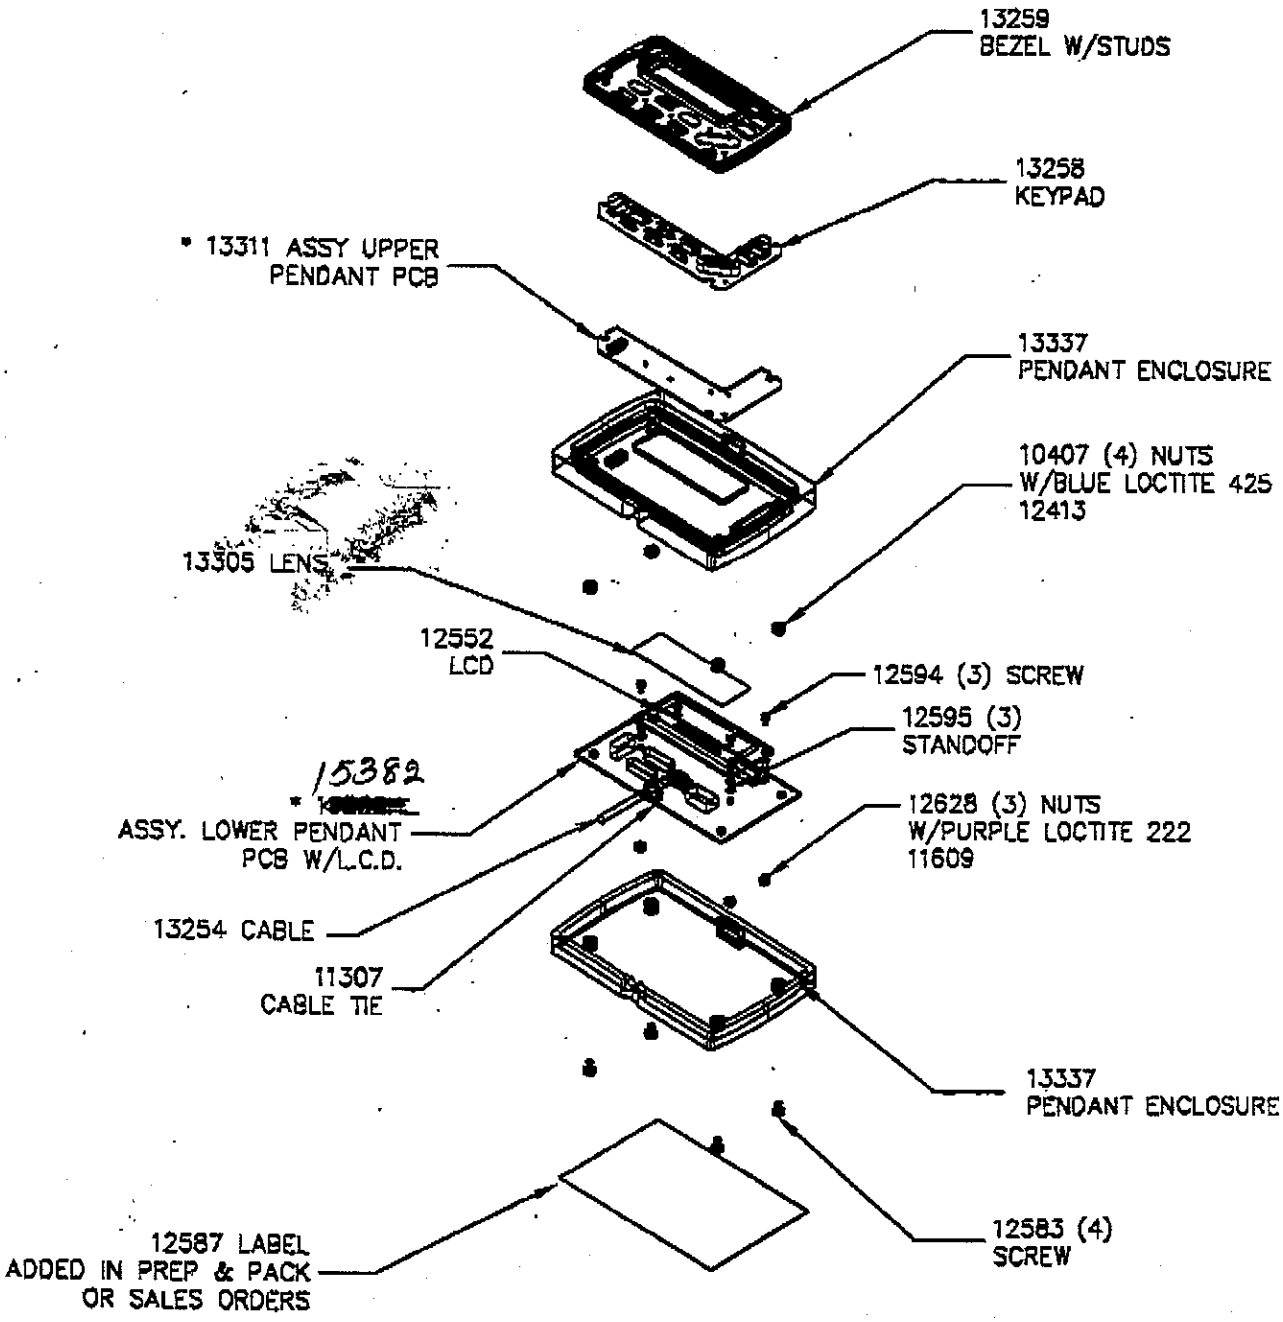
13259
BEZEL W/STUDS
13258
KEYPAD
* 13311 ASSY UPPER
PENDANT PCB
13337
PENDANT ENCLOSURE
10407 (4) NUTS
W/BLUE LOCTITE 425
12413
13305 LENS
12552
LCD
12594 (3) SCREW
12595 (3)
STANDOFF
15382
* [redacted]
ASSY. LOWER PENDANT
PCB W/L.C.D.
12628 (3) NUTS
W/PURPLE LOCTITE 222
11609
13254 CABLE
11307
CABLE TIE
13337
PENDANT ENCLOSURE
12587 LABEL
ADDED IN PREP & PACK
OR SALES ORDERS
12583 (4)
SCREW

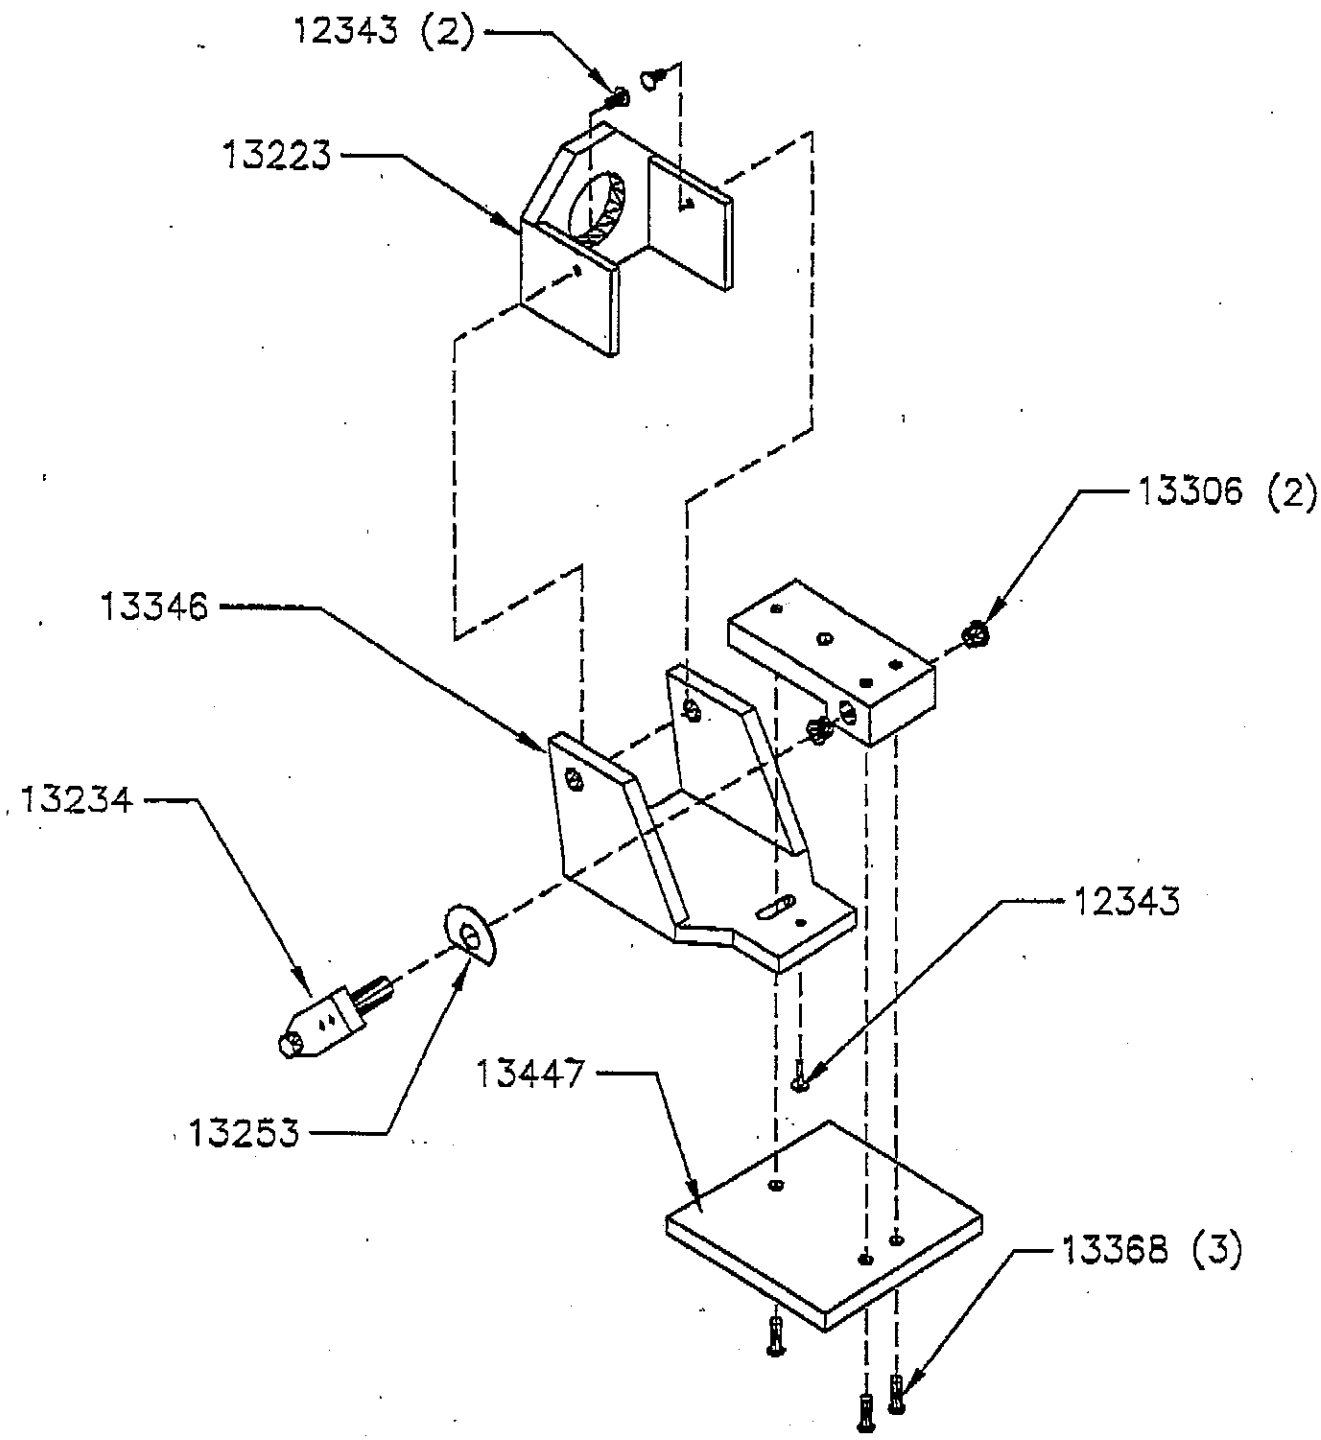
12343 (2)
13223
13306 (2)
13346
13234
12343
13447
13253
13368 (3)